



Summary of Results:


Vacuum Bead Technology in the VACOcast Diabetic provides equal ankle stability as in a fresh cast

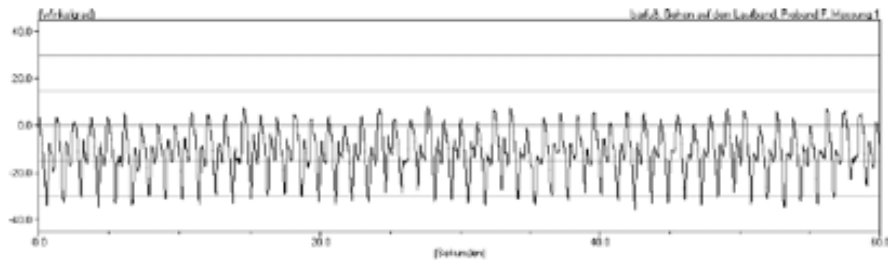

Shoe

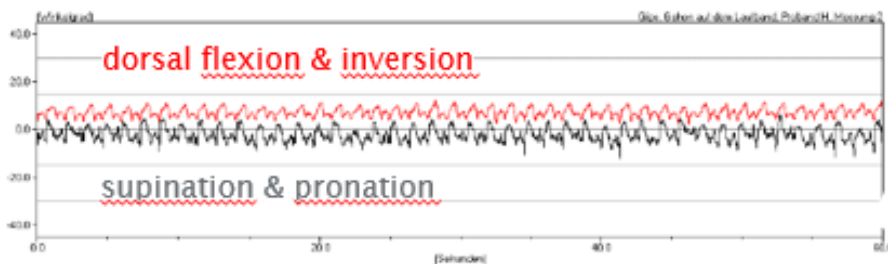

Fresh Cast

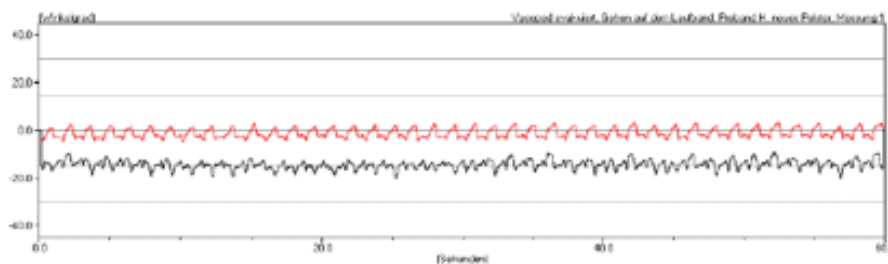

Vacuum Bead Technology

Amplitude in the ankle joint movement while stair climbing (electronic goniometer)